



Properties of Acrylic Resin For CAD/CAM: A Systematic Review and Meta-Analysis of In Vitro Studies

Emanuele de Oliveira, DDS ¹, Elisa Zancanaro de Figueiredo, DDS, MSc ¹, Ana Maria Spohr, DDS, MSc, PhD,² & Márcio Lima Grossi, DDS, MSc, PhD¹

¹Post-Graduate Program in Dentistry (Prosthodontics), School of Health and Life Sciences, Pontifical Catholic University of Rio Grande do Sul (PUCRS), Porto Alegre, Brazil

²Post-Graduate Program in Dentistry (Restorative Dentistry), School of Health and Life Sciences, Pontifical Catholic University of Rio Grande do Sul (PUCRS), Porto Alegre, Brazil

Keywords

Complete denture; acrylic resin; CAD/CAM; poly(methylmethacrylate).

Correspondence

Emanuele de Oliveira, Post-Graduate Program in Dentistry (Prosthodontics), School of Health and Life Sciences, Pontifical Catholic University of Rio Grande do Sul (PUCRS), Ipiranga Avenue 6681, Porto Alegre, RS 90619-900, Brazil.

E-mail: emanuele_o@outlook.com

Funding: This work was supported by the Coordenação de Aperfeiçoamento de Pessoal de Nível Superior (CAPES) – Brazil – Finance code 001.

Accepted May 19, 2021

doi: 10.1111/jopr.13394

Abstract

Purpose: This systematic review and meta-analysis of in vitro studies compared the prepolymerized acrylic resin used for CAD/CAM complete denture manufacturing versus the heat-polymerized acrylic resin for conventional complete dentures in terms of surface roughness, wettability, hardness and flexural strength.

Materials and Methods: An electronic search was performed in the PubMed, Embase, LILACS and Web of Science databases, without language or date restrictions. Gray literature and manual search tools were also used. The systematic review was carried out by two researchers independently, following the inclusion criteria: in vitro studies testing the CAD/CAM acrylic resin with a control group of heat-polymerized acrylic resin which compared at least one of the four material properties above. The meta-analysis was performed separately for each property, using a random effect model.

Results: Of the 914 studies found by means of search strategies, 698 were selected for the systematic review. After applying the eligibility criteria, only 17 articles were selected for the qualitative analysis in the systematic review; among these, 14 were included in the quantitative meta-analysis. The CAD/CAM prepolymerized acrylic resin in blocks had similar properties when compared to heat-polymerized acrylic resin in almost all outcome measures, with the exception of a statistically significant reduction in surface roughness.

Conclusions: Based on the findings of this systematic review and meta-analysis, equally satisfactory results can be expected from dental prosthesis manufactured by the CAD/CAM system when compared to conventional ones, with the additional potential of reducing the pigmentation and attached microorganisms due to the reduced surface roughness of the prepolymerized resin.

The poly(methylmethacrylate) (PMMA) based heat-polymerized acrylic resin has become the material of choice for manufacturing complete dentures (CDs) since its introduction in the dental market. Due to its favorable properties, its use is widespread and popular in complete oral rehabilitations.^{1,2}

Properties like wettability and surface roughness can impact the esthetic results and quality of life for wearers of CDs. Esthetics can be compromised by the impregnation of pigments to the prosthesis acrylic base, when the material properties are not adequate. In addition, these acrylic resin properties play a major role in the accumulation and colonization of microorganisms that may lead to denture stomatitis and halitosis.^{2,3}

During mastication, dentures are subjected to flexural or bending forces, which induce stress in the acrylic base and re-

sults in internal tensions or even small cracks. The propagation of these cracks over time might lead to the prosthesis fracture. The predisposition to fracture is also determined by alterations in the prosthesis base, wearing of the teeth, and change in the supporting tissues.^{4,5} For this reason, it is important for the material to have an adequate flexural strength, considering that the alveolar resorption is a process that occurs gradually and irregularly, which might lead to an imbalance and mismatch in the prosthesis support by the hard and soft tissues.⁶ The denture's resistance to grinding is determined by the hardness of the acrylic resin material.^{7,8}

The CAD/CAM technology was introduced in the manufacturing of CDs by Maeda et al.⁹ The objective of this digital approach is: to reduce the number of consultations to two or three

appointments, to facilitate the duplication of existing prostheses, to optimize the prosthesis precision and to improve its mechanical properties.¹⁰ The prosthetic bases are milled from blocks of preheated acrylic resin, where the polymerization process occurs under standardized conditions, which in turn reduces the possibility of operator interferences. The lack of control over the polymerization rate as well as the incorporation of cracks and porosities during the conventional heated acrylic polymerization may worsen mechanical properties.⁴ Regarding the industrial processing, the formation of polymer chains and the degree of conversion from monomers to polymers are higher, resulting in lower levels of residual monomers and polymerization contraction.^{7,11,12}

Taking into consideration that the manufacturing of removable CDs is still a common practice, and that the long-term performance is directly related to the material properties, a review of the literature might help health professionals to inform their choices regarding materials and techniques. Thus, this *in vitro* systematic review and meta-analysis has the objective of comparing the prepolymerized acrylic resin for CAD/CAM CDs versus the heat-polymerized acrylic resin for conventional CDs in terms of surface roughness, wettability, hardness and flexural strength. The null hypothesis tested was that there is no difference between CAD/CAM acrylic resin and heat-polymerized acrylic resin.

Materials and methods

This systematic review and meta-analysis was based on the Preferred Reporting Items for Systematic Review and Meta-Analysis (PRISMA) guidelines and the research protocol is registered in the PROSPERO database (ID CRD42020157053).¹³ The research question: “Does the CAD/CAM acrylic resin possess similar properties to the heat-polymerized acrylic resin?”, was formulated according to the PICOS model, where “P” is the population (i.e., removable partial denture), “I” is the intervention group (i.e., acrylic resin for CAD/CAM prosthesis), “C” is the comparison group (i.e., heat-polymerized acrylic resin for conventional prosthesis), “O” is the outcome (i.e., surface roughness, wettability, hardness and flexural strength); and “S” is the study design (i.e., *in vitro* studies).¹⁴

The search strategy used controlled and non-controlled descriptors as well as Boolean terms (OR, AND). The search in PubMed, Embase, LILACS and Web of Science databases was performed without language or year restrictions. The articles were searched in PubMed/MEDLINE using the following terms: (“Denture, Complete” [mesh] OR “Complete Denture” OR “Complete Dentures” OR “Dentures Complete”) AND (“Computer-Aided Design” [mesh] OR “Computer Aided Design” OR “Computer-Aided Designs” OR “Design, Computer-Aided” OR “Designs, Computer-Aided” OR “Computer-Assisted Design” OR “Computer Assisted Design” OR “Computer-Assisted Designs” OR “Design, Computer-Assisted” OR “Designs, Computer-Assisted” OR “Computer-Aided Manufacturing” OR “Computer Aided Manufacturing” OR “Manufacturing, Computer-Aided” OR “Computer-Assisted Manufacturing” OR “Computer Assisted

Manufacturing” OR “Manufacturing, Computer-Assisted” OR “CAD-CAM”).

Literature search was also performed in the gray literature using the Brazilian Digital Library of Thesis and Dissertations (BDTD), Google Scholar, and OpenGrey. In addition, the references of selected studies were also manually searched and included when applicable. Finally, specialized journals from the field of interest were searched from 1994 until the present time (*Journal of Prosthodontics*, *Dental Materials*, *International Journal of Prosthodontics*, and *Journal of Prosthetic Dentistry*).

The results of the database search were exported to the End-Note web program (Clarivate Analytics, PA), where the exclusion of duplicated articles was performed. After the study selection, a two-phase selection was carried out by two independent researchers (one master and one doctoral student). The first phase was characterized by reading of titles and abstracts, where the article was included by at least one researcher. The second phase was characterized by full text reading, and the articles inclusion or exclusion had to be agreed to by both researchers. In case of disagreement, a third evaluator was consulted to make the final decision (graduate students’ supervisor).

The inclusion criteria were: *in vitro* studies testing the CAD/CAM acrylic resin versus the conventional heat-polymerized acrylic resin control group, evaluating at least one of the four properties of this study (i.e., surface roughness, wettability, hardness and flexural strength). Other acrylic resin properties which were not part of the inclusion criteria were considered part of the exclusion criteria (e.g., non *in vitro* studies or *in vitro* studies without a control group). For data extraction, a standardized Excel software spreadsheet was created and completed by the researchers.

The evaluation of the methodological quality of the studies, carried out by two independent researchers, was based in the items set forth by the Consolidated Standards of Reporting Trials (CONSORT).¹⁵

The statistical program used for data analysis and graphic production was the RStudio version 1.2.5019 (Meta package version 4.11-0).¹⁶ The heterogeneity was assessed by means of the I^2 inconsistency test, which attributed a value from 0% to 100%, which shows how much the magnitude of difference among studies can be explained by heterogeneity, and not by chance. From 0 to 25% was considered a low heterogeneity; from 25% to 75%, intermediate heterogeneity; and from 75% or higher, high heterogeneity.¹⁷

If the comparison among the selected studies was possible, the data were analyzed quantitatively in a meta-analysis using forest plot graphs. Considering that the outcomes are continuous variables, the measure of effect was analyzed using mean deviations. Depending on the heterogeneity, either the random effect model (REM) or the fixed effect model (FEM), or both, were used at a 5% statistical significance.¹⁸

Results

The fluxogram including the identification and selection of the studies as well as the reasons for the exclusion are shown in Figure 1. The electronic search yielded 914 articles, and after

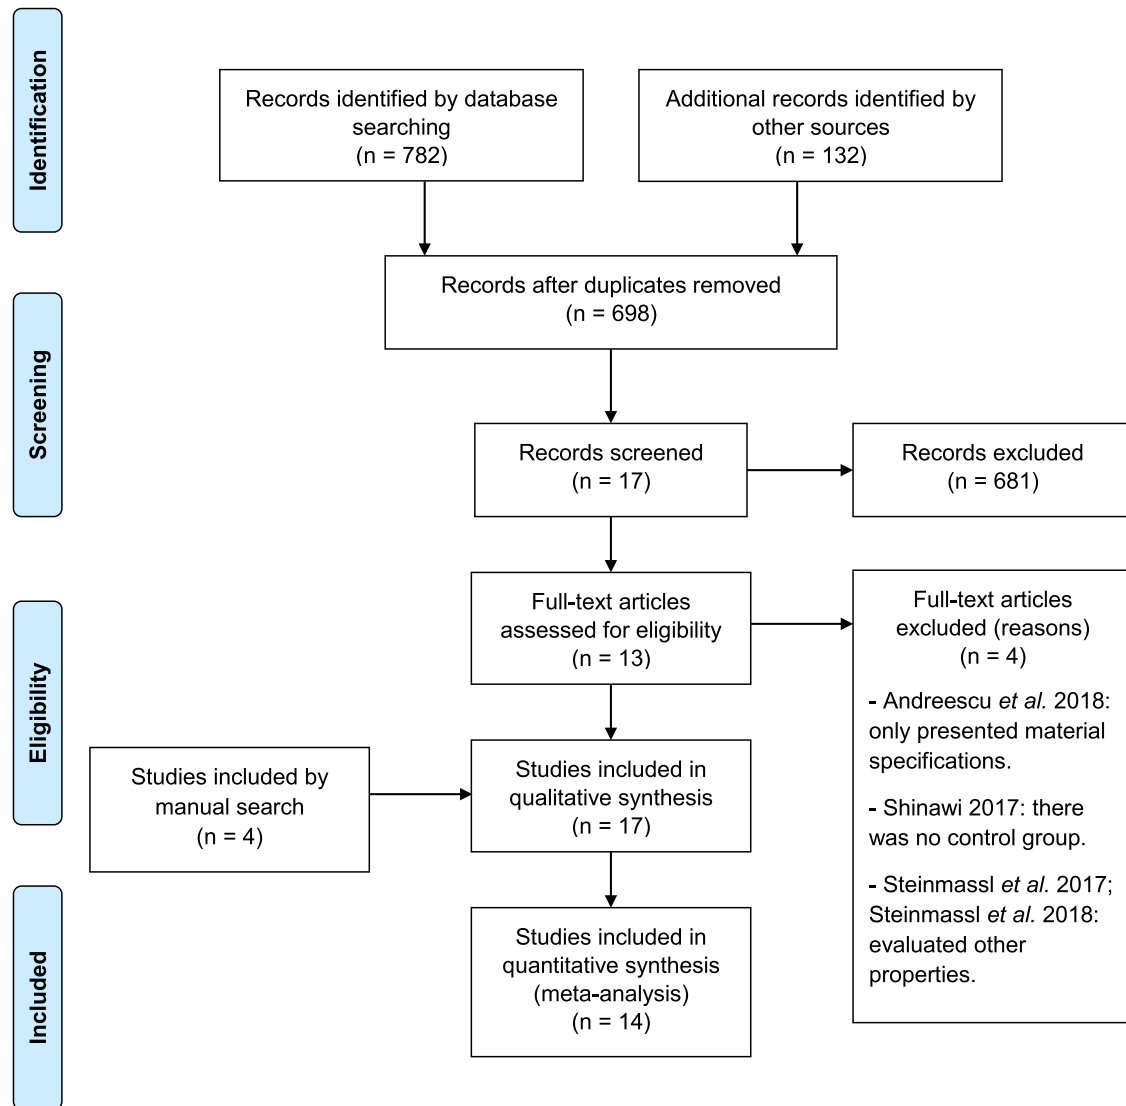


Figure 1 PRISMA Flow diagram of article selection.

the removal of duplications, 698 articles were selected for further analysis. After title and abstract reading, 17 articles were selected for full-text reading, four of which were excluded and 13 remained (Fig 1). On the other hand, four new articles were added by means of manual search, resulting in 17 articles to be included in the qualitative analysis (i.e., systematic review). The study description of each article is shown in Table 1 (i.e., authorship, year of publication, material properties evaluated, tests used, sample size, etc.). As there were no language restrictions, articles written in Turkish²⁹ and Portuguese³⁰ were included.

Out of the 17 articles selected for the systematic review, only 14 were selected for the meta-analysis for presenting comparable values and methodologies. Therefore, the following studies were excluded from the quantitative analysis: Alp *et al.*²⁰ and Murat *et al.*²¹ who showed the test results only after thermal

cycling; and Al-Fouzan *et al.*,²⁵ who showed surface roughness in terms of area values (Sa), which could not be compared with the other studies that displayed surface roughness using mean values (Ra). The three excluded studies were only analyzed qualitatively (Table 1).

The qualitative analysis of the studies is described in Table 2. Considering that CONSORT¹⁵ items 6, 7, 8, and 14 do not apply to *in vitro* studies and considering that they were designed for randomized clinical trials (RCT), only the remaining items were taken into consideration in the evaluation (i.e., 11 items). In general, all studies showed satisfactory quality, fulfilling at least 7^{7,23} to a maximum of 10²⁷ out of 11 analyzed items.

In the meta-analysis, only studies which showed mean and standard deviation for both experimental and control groups and which used the same units of comparison for the four material properties considered in the present study were

Table 1 General description of the selected studies for the systematic review (qualitative analysis)

First author and year	Evaluated properties	Tests	Sample size (n)	Dimensions	Storage	ISO	Unit
Aguirre, 2020 ¹⁹	Flexural strength	Three-point bending test	10	63×10×3.3 mm	Distilled water at 37°C for 7 days	20795-1	MPa
Alp, 2019 ²⁰	Flexural strength	Three-point bending test	15	25×2×2 mm	Distilled water at 37°C for 24 hours	10477: 2004	MPa
Murat, 2019 ²¹	Surface roughness Wettability	Contact profilometer Contact angle measurement	10	10×2 mm	Distilled water for 6 days	NR	μm degree
Pacquet, 2019 ¹²	Hardness	Vickers hardness	10 (H)	65×10×2.5 mm	Distilled water at 37°C for 24 hours	20795-1	HV MPa
Alammari, 2017 ²²	Flexural strength Surface roughness Wettability	Three-point bending test Profilometer Contact angle measurement	25 (FS) 10	30×15×3 mm	Distilled water at room temperature for 24 hours	NR	μm degree
Al-Dwairi, 2020 ⁴	Flexural strength	Three-point bending test	15	65×10×3 mm	Distilled water at 37°C for 7 days	1567	MPa
Ayman, 2017 ⁷	Flexural strength	Three-point bending test	10	65×10×3 mm	Distilled water at 37°C for 24 hours	NR	MPa
Perea-Lowery, 2020 ²³	Hardness Flexural strength	Vickers hardness Three-point bending test	8	10×10×2 mm (H) 65×10×3.2 mm (FS)	Distilled water at 37°C for 30 days	1567	HV MPa
Srinivasan, 2018 ²⁴	Surface roughness	Non-contact profilometer	5	20×20×1.5 mm	70% ethanol solution for 5 minutes and drying with sterile cotton	11562	μm
Al-Dwairi, 2019 ²	Surface roughness Wettability Hardness	Contact profilometer Contact angle measurement Vickers hardness	15	25×25×3 mm	Distilled water for 48 hours	NR	μm degree HV
Al-Fouzan, 2017 ²⁵	Surface roughness	Non-contact profilometer	10	10×3 mm	NR	NR	μm
Alp, 2019 ²⁶	Surface roughness	Contact profilometer	6	10×2×2 mm	Ultrasound cleaning in distilled water for 10 minutes and drying with paper towel	NR	μm
Arslan, 2018 ⁶	Surface roughness Wettability Flexural strength	Contact profilometer Contact angle measurement	10	64×10×3.3 mm	Water at 37°C for 48 hours	20795-1	μm degree MPa
Bedrossian, 2019 ²⁷	Flexural strength	Three-point bending test	16	32×10×3 mm	Water at 37°C for 50 hours	20795-1	MPa
Steinmassl, 2018 ²⁸	Surface roughness Wettability	Contact profilometer Contact angle measurement	10	39×8×4 mm	Deionized water at 21°C for 7 days in darkness	3274	μm degree
Dayan, 2019 ²⁹	Hardness	Vickers hardness	8	15×2 mm	Distilled water at 37°C for 24 hours	NR	HV
Costa, 2018 ³⁰	Surface roughness	Contact profilometer	10	12×12×3 mm	Deionized water at 37°C for 24 hours	NR	μm

NR = not reported.

Table 2 Risk of bias of the selected studies from the databases and gray literature for the meta-analysis

Author (year)	1	2a	2b	3	4	5	6	7	8	9	10	11	12	13	14
Aguirre et al, 2020 ¹⁹	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	Yes	No	No
Pacquet et al, 2019 ¹²	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	No	Yes	No
Alammari, 2017 ²²	Yes	Yes	Yes	Yes	Yes	Yes	No	No	No	No	Yes	Yes	No	No	No
Al-Dwairi et al, 2020 ⁴	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	Yes	Yes	No
Ayman, 2017 ⁷	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	No	No	No
Perea-Lowery et al, 2020 ²³	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	No	No	No
Srinivasan et al, 2018 ²⁴	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	Yes	Yes	No
Al-Dwairi et al, 2019 ²	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	No	Yes	No
Alp et al, 2019 ²⁶	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	Yes	Yes	No
Arslan et al, 2018 ⁶	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	Yes	No	No
Bedrossian et al, 2019 ²⁷	Yes	Yes	Yes	Yes	Yes	Yes	No	No	No	No	Yes	Yes	Yes	Yes	No
Steinmassl et al, 2018 ²⁸	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	No	Yes	No
Dayan, 2019 ²⁹	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	Yes	No	No
Costa, 2018 ³⁰	Yes	Yes	Yes	Yes	Yes	No	No	No	No	No	Yes	Yes	Yes	Yes	No

(1) Structured summary of trial design, methods, results, and conclusions; (2a) Scientific background and explanation of rationale; (2b) Specific objectives and/or hypotheses; (3) The intervention for each group, including how and when it was administered, with sufficient detail to enable replication; (4) Completely defined, pre-specified primary and secondary measures of outcome, including how and when they were assessed; (5) How sample size was determined; (6) Method used to generate the random allocation sequence; (7) Mechanism used to implement the random allocation sequence; (8) Who generated the random allocation sequence; (9) If done, who was blinded after assignment to intervention; (10) Statistical methods used to compare groups; (11) Results for each group, and the estimated size of the effect and its precision (for example, 95% confidence interval); (12) Trial limitations, addressing sources of potential bias, imprecision, and, if relevant, multiplicity of analyses; (13) Sources of funding and other support; (14) Where the full trial protocol can be accessed, if available.

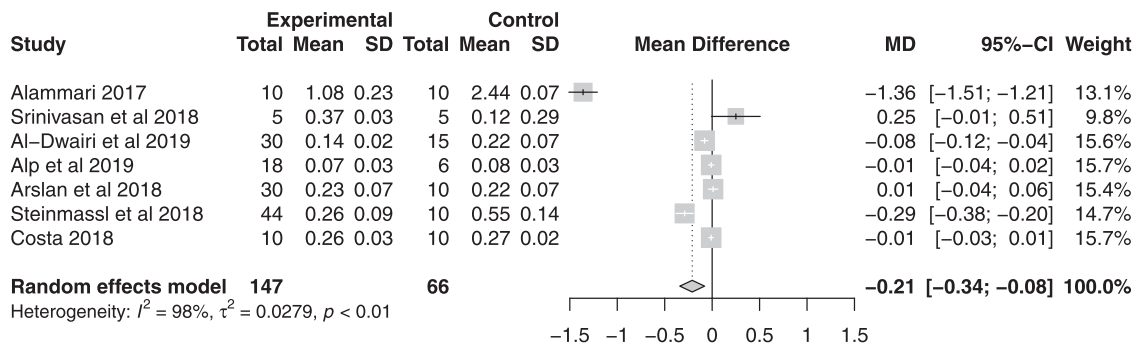


Figure 2 Forest plot: surface roughness, experimental (CAD/CAM) and control (heat-polymerized) acrylic resin groups. SD = standard deviation; CI = confidence interval.

included. Quantitative analysis was divided according to each material property evaluated: surface roughness (Fig 2), wettability (Fig 3), hardness (Fig 4) and flexural strength (Fig 5).

Figure 2 shows the forest plot graph of the meta-analysis among the studies^{2,6,22,24,26,28,30} which evaluated the materials surface roughness by means of a profilometer. The analysis resulted in a statistically significant reduction of the surface roughness of CAD/CAM acrylic resin ($p < 0.001$) in comparison to the heat-polymerized acrylic resin for conventional CDs.

Wettability

Figure 3 shows the forest plot graph of the meta-analysis among the studies^{2,6,22,28} which evaluated the acrylic resin wettability of both materials, with the measurement of contact angle of the drop with the acrylic resin surface. The analysis

showed no statistically significant difference ($p = 0.861$) between the experimental and control materials studied.

Hardness

Figure 4 shows the forest plot graph generated by the meta-analysis among the studies^{2,12,23,29} which evaluated the acrylic resin hardness between the two materials by means of the Vickers hardness test. No statistically significant difference ($p = 0.615$) was found between the CAD/CAM versus conventional acrylic resin.

Flexural strength

Figure 5 displays the forest plot graph from the meta-analysis among the studies^{4,6,7,12,19,23,27} which compared both acrylic resin flexural strength by using a 3-point bend test. No

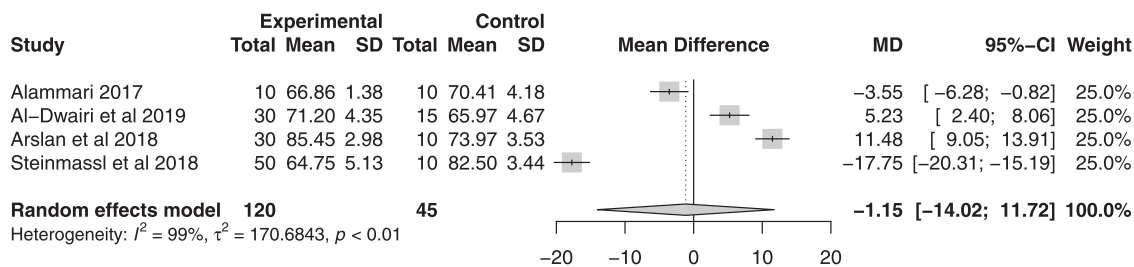


Figure 3 Forest plot: wettability, experimental (CAD/CAM) and control (heat-polymerized) acrylic resin groups. SD = standard deviation; CI = confidence interval.

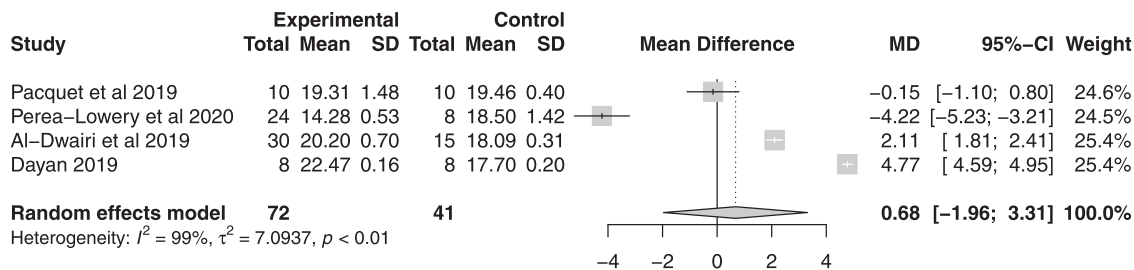


Figure 4 Forest plot: hardness, experimental (CAD/CAM) and control (heat-polymerized) acrylic resin groups. SD = standard deviation; CI = confidence interval.

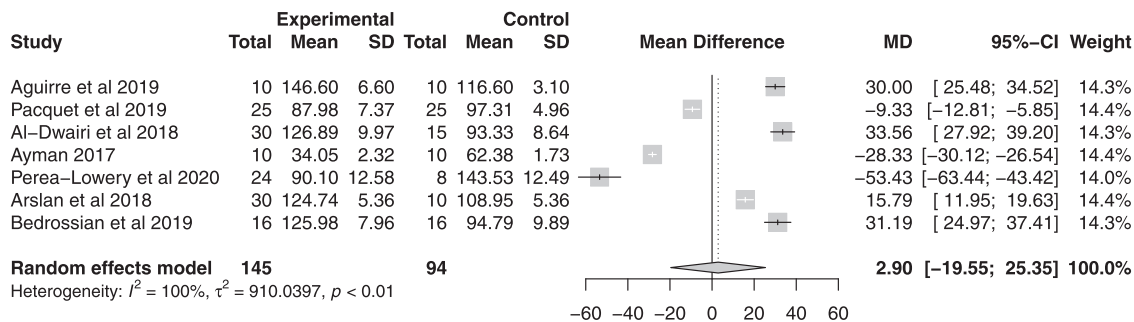


Figure 5 Forest plot: flexural strength, experimental (CAD/CAM) and control (heat-polymerized) acrylic resin groups. SD = standard deviation; CI = confidence interval.

statistically significant difference ($p = 0.800$) was found between the two materials analyzed.

Discussion

The acrylic resin blocks used in the CAD/CAM systems are prepolymerized under specific and standardized conditions; and because of that, it is believed that it has improved material properties when compared to the heat-polymerized acrylic resin for conventional CDs.^{2,4} In this study, no statistically significant differences were found in wettability, hardness and flexural strength between the two acrylic resins assessed. Only surface roughness was significantly better in the CAD/CAM prepolymerized acrylic resin. Thus, the null hypothesis of this study was partially accepted.

Regarding the methodological characteristics of the studies included in this systematic review, it was verified that most authors reported the ISO norms in which they based the manufacturing of their test samples and protocols. The test norms and protocols are specific for prosthesis base polymers. It is important to point out that the ISO 1567 norm³¹ has not been valid since 2008, and it was later replaced by the current 20795-1 norm³²; however, some authors still refer to the outdated norm.^{4,23} The ISO 11562³³ and 3274³⁴ norms deal with geometric specifications, specifically the material's surface texture. It could be observed also that the selected studies keep, in general, a standard regarding sample size, where the majority of them had 10 samples per group (range = 5 to 25).

The microbial adhesion is determined by surface roughness, where the increase in roughness between 0.1 and 0.4 μm implies an increase in the colonization of microorganisms.²⁸ A

threshold surface roughness of $0.2 \mu\text{m}$ (Ra) indicates a maximum acceptable value,³⁵ below which no further reduction in bacterial accumulation could be expected. The adoption of an effective protocol of finishing and polishing of the prosthesis surface is essential and contributes to the increase in surface smoothness. However, the finishing and refined polishing is only indicated in the external surface of the CDs, because the internal surface must be preserved to remain in the closest possible contact to the remaining tissues.

All authors used some form of mechanical polishing of the samples before the tests, mimicking the protocol that occurs in daily clinic.²² In this stage, authors used grinding points and silicon carbide papers, which varied from 120 to 1,200 grits.

Physical properties of conventional heat-polymerized acrylic resins are influenced by different factors, such as: size of the polymer spheres in the resin powder, type of initiator and accelerator,³⁶ and aspects related to the prosthesis technician who performs the acrylic processing (i.e., powder/liquid proportion and thermal cycle).²² Despite the fact that the chemical composition seems to have an important role in the determination of the material properties, the processing protocol is the main determinant of the surface roughness.²⁸ The improved surface roughness of the prepolymerized CAD/CAM acrylic resin might be attributed to the manufacturing process exclusive of these materials.

The wettability is the indicator of the saliva and other fluids capacity to spread over a surface. The contact angle is considered the result of the balance between the interfacial and surface forces.² Small contact angles represent a greater hydrophilicity, which is fundamental in the retention of removable prosthesis, but also favors the staining and adhesion of microorganisms² as well as the composition of the biofilm.²⁸

Al-Dwairi *et al*² and Arslan *et al*⁶ found a greater hydrophobicity in the CAD/CAM acrylic resin, while Alammari²² and Steinmassl *et al*²⁸ found more hydrophilicity for CAD/CAM resins. The results of this study showed no statistical difference regarding the wettability of either acrylic resins. We can expect prosthesis manufactured with the CAD/CAM system to have an adequate retention, due to the formation of a saliva film over the prosthesis, with the potential of reducing the pigmentation and attached microorganisms due to the reduced surface roughness.

The hardness refers to the material density as well as its resistance to wearing and/or abrasion. This property affects the mechanical behavior and durability of the prosthesis during function, parafunction, and cleaning methods used over time.⁷ It is also considered an indirect method to evaluate the degree of monomeric conversion obtained, and as a result, the quality of the polymerization reaction. Higher hardness values indicate better polymerization with higher degree of monomeric conversion of acrylic resins.³⁷

The association of higher-pressure values and temperature yield an increase in the degree of monomeric conversion of acrylic resins, reducing the concentration of residual monomer and forming polymers with higher molecular weight and longer chains.²³ In this manner, with closer chains among themselves, the material becomes denser. The hardness test also helps to predict the mechanical behavior of base resins

for prosthesis, correlating with the flexural properties that the material presents.³⁸

The flexural strength can be considered one of the most important mechanical properties of the acrylic prosthesis. Testing the materials to flexural strength by using a 3-point bend test simulates its capacity to resist to high functional loads during mastication or parafunction.^{19,27} According to the specifications of ISO 20795-1 norm³² for prosthesis base polymers, the value of flexure strength obtained in acrylic resins type 1 should not be less than 65MPa. In the included studies, it was verified that in most of the acrylic resins, both prepolymerized acrylic resin for fabricating CAD/CAM CDs and the heat-polymerized acrylic resin for conventional CDs, fulfill this requirement. Clinically, the use of material for prosthesis base with higher flexural strength makes the prosthesis less prone to fracture.¹⁹

Alp *et al*²⁰ and Murat *et al*²¹ were not included in the meta-analysis, because they only showed data after the thermal cycling. Both authors performed 10,000 thermal cycles in their samples in order to simulate one year of physiological aging. These authors described statistically significant differences between CAD/CAM versus conventional acrylic resins in flexural strength, with superior values in the prepolymerized resin (i.e., CAD/CAM). Besides a smaller surface roughness and contact angle in the CAD/CAM samples, they also reported a greater adhesion of *Candida albicans* in the thermopolymerized acrylic resins. Studies which adopted the aging methodology are of great importance, because they indicate that the good mechanical behavior of prepolymerized acrylic resins remain effective over time in oral conditions. This is paramount when patients use removable prosthesis for long periods of time.

The lack of meta-analysis of samples aged in the laboratory can be considered a limitation of this study. It is due to the absence of a greater number of studies which tested this methodology before and after the use of thermocycling, which allows a more reliable comparison and estimation of the behavior of these samples over time. Therefore, future studies should include aged samples in their experiments. Also, the high heterogeneity observed in all analysis can be considered an intrinsic limitation of *in vitro* studies; these studies are very precise and show a very small standard deviation, making the heterogeneity more easily identified.

The inclusion of digital technologies in the dental practice is a trend worldwide. The replacement of analogic for digital processing has been taking place in a gradual manner, and despite being in its initial stage, the milling of CAD/CAM CDs show promising results. Studies have shown retention^{39,40} and precision⁴¹ results significantly better in CAD/CAM CDs than in conventional ones, with good levels of patient satisfaction,⁴² esthetics and phonetics.⁴³

Conclusion

The prepolymerized acrylic resin in blocks for CAD/CAM show similar properties to thermoheated ones, with additional reduction in surface roughness, and it can be considered a potential alternative to conventional CDs.

Conflict of interest statement

The authors report no conflicts of interest.

References

1. Parvizi A, Lindquist T, Schneider R, et al: Comparison of the dimensional accuracy of injection-molded denture base materials to that of conventional pressure-pack acrylic resin. *J Prosthodont* 2004;13:83-89
2. Al-Dwairi ZN, Tahboub KY, Baba NZ, et al: A comparison of the surface properties of CAD/CAM and conventional polymethylmethacrylate (PMMA). *J Prosthodont* 2019;28:452-457
3. Susewind S, Lang R, Hahnel S: Biofilm formation and *Candida albicans* morphology on the surface of denture base materials. *Mycoses* 2015;58:719-727
4. Al-Dwairi ZN, Tahboub KY, Baba NZ, et al: A comparison of the flexural and impact strengths and flexural modulus of CAD/CAM and conventional heat-cured polymethyl methacrylate (PMMA). *J Prosthodont* 2020;29:341-349
5. Beyli MS, Von Fraunhofer JA: An analysis of causes of fracture of acrylic resin dentures. *J Prosthet Dent* 1981;46:238-241
6. Arslan M, Murat S, Alp G, et al: Evaluation of flexural strength and surface properties of prepolymerized CAD/CAM PMMA-based polymers used for digital 3D complete dentures. *Int J Comput Dent* 2018;21:31-40
7. Ayman AD: The residual monomer content and mechanical properties of CAD\CAM resins used in the fabrication of complete dentures as compared to heat cured resins. *Electron Physician* 2017;9:4766-4772
8. Murakami N, Wakabayashi N, Matsushima R, et al: Effect of high-pressure polymerization on mechanical properties of PMMA denture base resin. *J Mech Behav Biomed Mater* 2013;20:98-104
9. Maeda Y, Minoura M, Tsutsumi S, et al: A CAD/CAM system for removable denture. Part I: fabrication of complete dentures. *Int J Prosthodont* 1994;7:17-21
10. Bidra AS, Taylor TD, Agar JR: Computer-aided technology for fabricating complete dentures: systematic review of historical background, current status, and future perspectives. *J Prosthet Dent* 2013;109:361-366
11. Infante L, Yilmaz B, McGlumphy E, et al: Fabricating complete dentures with CAD/CAM technology. *J Prosthet Dent* 2014;111:351-355
12. Pacquet W, Benoit A, Hatège-Kimana C, et al: Mechanical properties of CAD/CAM denture base resins. *Int J Prosthodont* 2019;32:104-106
13. Moher D, Shamseer L, Clarke M, et al: Preferred reporting items for systematic review and meta-analysis protocols (PRISMA-P) 2015 statement. *Syst Rev* 2015;4:1
14. Moher D, Liberati A, Tetzlaff J, et al: Preferred reporting items for systematic reviews and meta-analyses: the PRISMA statement. *PLoS Med* 2009;6:e1000097
15. Faggion CM Jr: Guidelines for reporting pre-clinical in vitro studies on dental materials. *J Evid Based Dent Pract* 2012;12:182-189
16. General Package for Meta-Analysis. <https://cran.r-project.org/web/packages/meta/meta.pdf> . Accessed 6/7/2020
17. Higgins JP, Thompson SG, Deeks JJ, et al: Measuring inconsistency in meta-analyses. *BMJ* 2003;327:557-560
18. Analysing data and undertaking meta-analyses. <https://training.cochrane.org/handbook/current/chapter-10> . Accessed 6/7/2020
19. Aguirre BC, Chen JH, Kontogiorgos ED, et al: Flexural strength of denture base acrylic resins processed by conventional and CAD-CAM methods. *J Prosthet Dent* 2020;123:641-646
20. Alp G, Murat S, Yilmaz B: Comparison of flexural strength of different CAD/CAM PMMA-based polymers. *J Prosthodont* 2019;28:e491-e495
21. Murat S, Alp G, Alatalı C, et al: In vitro evaluation of adhesion of *Candida albicans* on CAD/CAM PMMA-based polymers. *J Prosthodont* 2019;28:e873-e879
22. Alammari MR: The influence of polishing techniques on pre-polymerized CAD\CAM acrylic resin denture bases. *Electron Physician* 2017;9:5452-5458
23. Perea-Lowery L, Minja IK, Lassila L, et al: Assessment of CAD-CAM polymers for digitally fabricated complete dentures. *J Prosthet Dent* 2021;125:175-181.
24. Srinivasan M, Gjengedal H, Cattani-Lorente M, et al: CAD/CAM milled complete removable dental prostheses: an in vitro evaluation of biocompatibility, mechanical properties, and surface roughness. *Dent Mater J* 2018;37:526-533
25. Al-Fouzan AF, Al-Mejrad LA, Albarrag AM: Adherence of *Candida* to complete denture surfaces in vitro: a comparison of conventional and CAD/CAM complete dentures. *J Adv Prosthodont* 2017;9:402-408
26. Alp G, Johnston WM, Yilmaz B: Optical properties and surface roughness of prepolymerized poly (methyl methacrylate) denture base materials. *J Prosthet Dent* 2019;121:347-352
27. Bedrossian EA, Chung KH, Ramos Jr V: Effect of layering gingiva-shade composite resin on the strength of denture base polymers. *J Prosthet Dent* 2019;122:153.e1-153.e8
28. Steinmassl O, Dumfahrt H, Grunert I, et al: Influence of CAD/CAM fabrication on denture surface properties. *J Oral Rehabil* 2018;45:406-413
29. Dayan S: Effect of various disinfection methods on the surface hardness of CAD/CAM and conventional acrylic resins. *Atatürk Üniversitesi Diş Hekimliği Fakültesi Dergisi* 2019;29:468-473
30. Costa RMB: Acrylic resin implemented in CAD-CAM technology: longitudinal and comparative analysis of surface roughness and microhardness after successive thermocycling cycles [dissertation]. Bauru, University of São Paulo, 2018
31. ISO 1567-1999 Dentistry — Denture base Polymers. <https://www.iso.org/standard/20266.html> . Accessed 8/9/2020
32. ISO 20795-1:2013 Dentistry — Base polymers — Part 1: denture Base Polymers. <https://www.iso.org/standard/62277.html>. Accessed 8/9/2020
33. ISO 11562:1996 Geometrical Product Specifications (GPS) — Surface texture: profile method — Metrological characteristics of phase correct filters. <https://www.iso.org/standard/21977.html>. Accessed 8/9/2020
34. ISO 3274:1996 Geometrical Product Specifications (GPS) — Surface texture: profile method — Nominal characteristics of contact (stylus) instruments. <https://www.iso.org/standard/1916.html>. Accessed 8/9/2020
35. Bollen CM, Papaioanno W, Van Eldere J, et al: The influence of abutment surface roughness on plaque accumulation and peri-implant mucositis. *Clin Oral Implants Res* 1996;7:201-211

36. Berger JC, Driscoll CF, Romberg E, et al: Surface roughness of denture base acrylic resins after processing and after polishing. *J Prosthodont* 2006;15:180-186
37. Soh MS, Yap AU: Influence of curing modes on crosslink density in polymer structures. *J Dent* 2004;32:321-326
38. Lee HH, Lee CJ, Asaoka K: Correlation in the mechanical properties of acrylic denture base resins. *Dent Mater J* 2012;31:157-164
39. AlHelal A, AlRumaih HS, Kattadiyil MT, et al: Comparison of retention between maxillary milled and conventional denture bases: a clinical study. *J Prosthet Dent* 2017;117:233-238
40. AlRumaih HS, AlHelal A, Baba NZ, et al: Effects of denture adhesive on the retention of milled and heat-activated maxillary denture bases: a clinical study. *J Prosthet Dent* 2018;120:361-366
41. Goodacre BJ, Goodacre CJ, Baba NZ, et al: Comparison of denture base adaptation between CAD-CAM and conventional fabrication techniques. *J Prosthet Dent* 2016;116:249-256
42. Saponaro PC, Yilmaz B, Johnston W, et al: Evaluation of patient experience and satisfaction with CAD-CAM-fabricated complete dentures: a retrospective survey study. *J Prosthet Dent* 2016;116:524-528
43. Neumeier TT, Neumeier H: Digital immediate dentures treatment: a clinical report of two patients. *J Prosthet Dent* 2016;116:314-319